

1/3

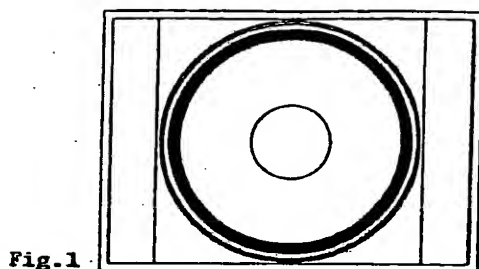


Fig. 1

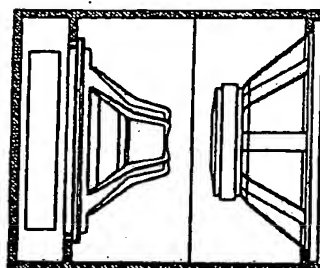


Fig. 1B

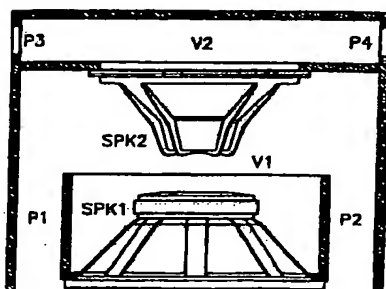


Fig. 1A

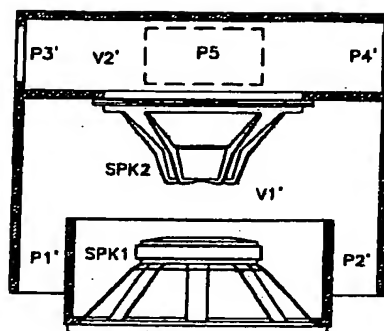


Fig. 2

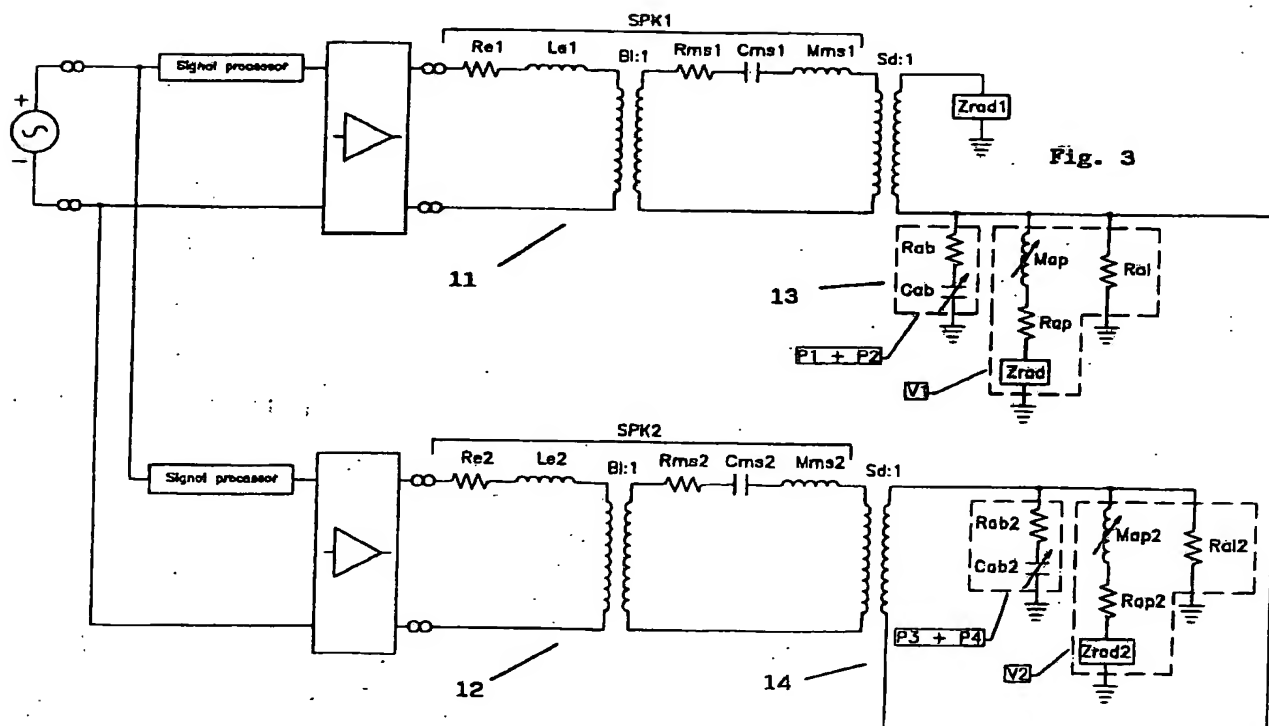


Fig. 3

# 2/3 Ratio vs Angle

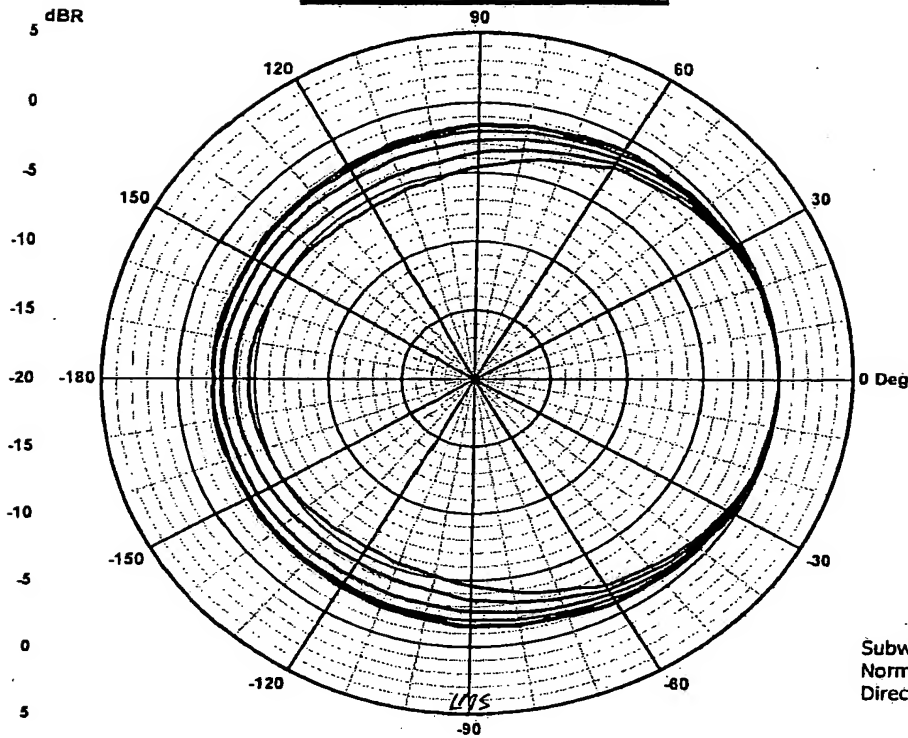


Fig. 4

Subwoofer System  
Normalized Polar Response Curve.  
Directivity Device OFF.

# Ratio vs Angle

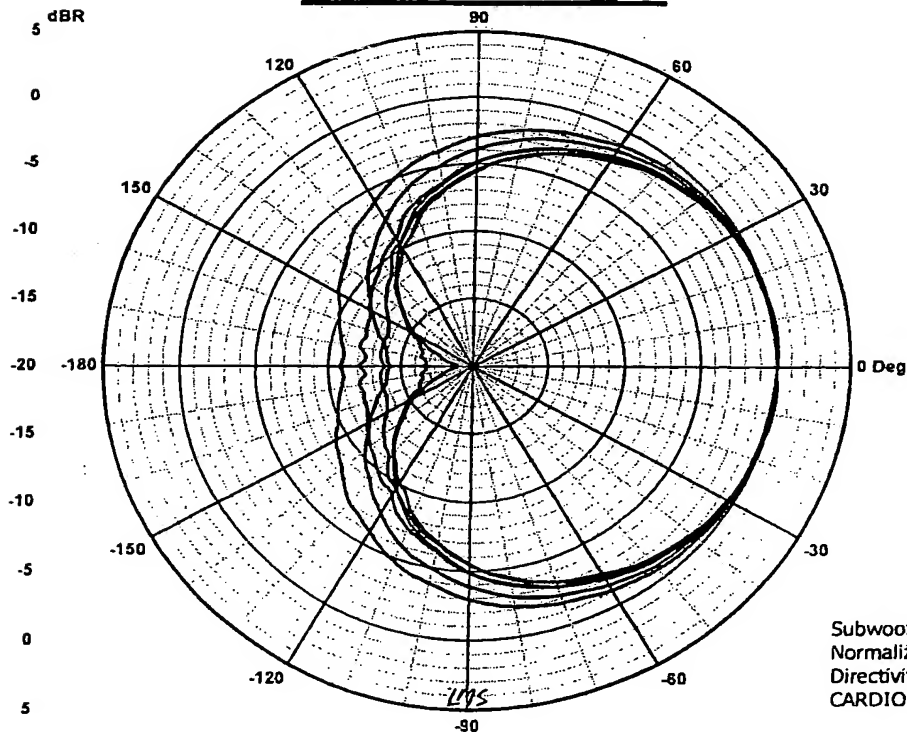


Fig. 5

Subwoofer System  
Normalized Polar Response Curves  
Directivity Device ON  
CARDIOIDLIKE RADIATION PATTERN

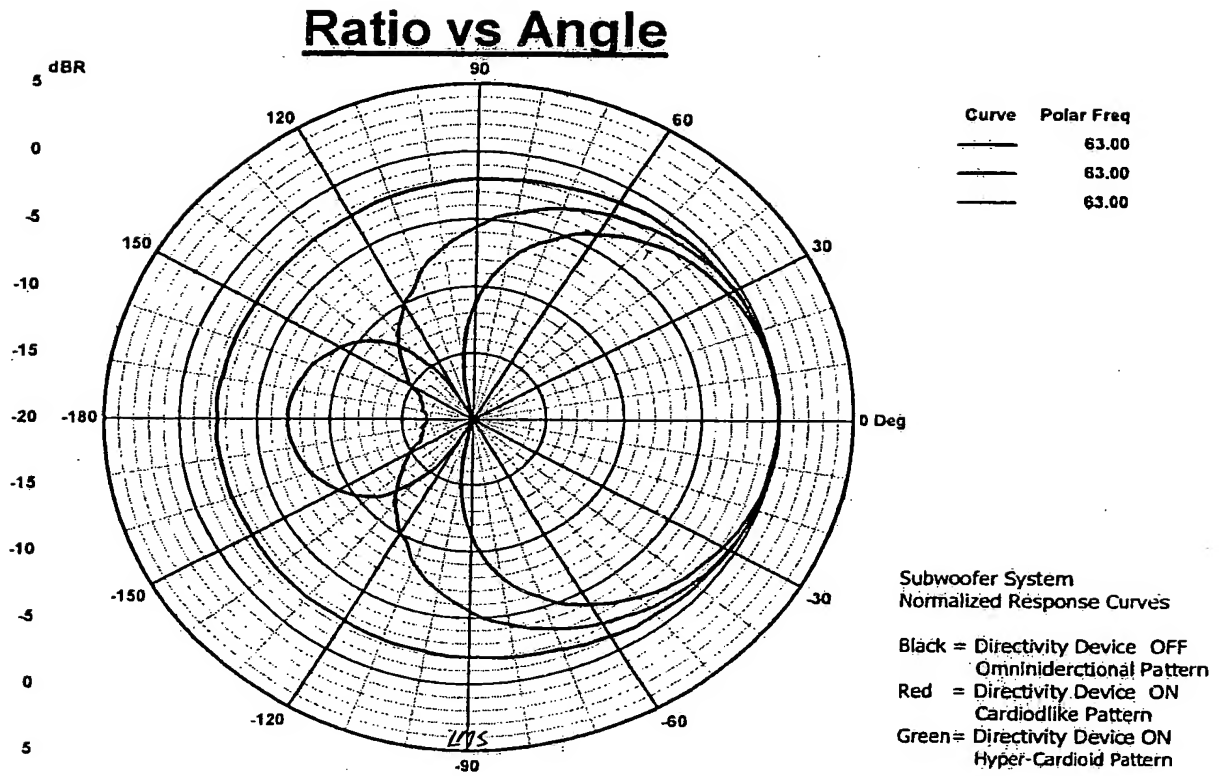


Fig. 6